

Development of a synchronous motion-tracking and video capture tool for flexible ureteroscopy

Jessica Trac¹, Jonguk Lee^{2,3}, Kai-Ho Fok^{4,5}, Brian Carrillo⁶, Monica Farcas^{4,5,7,8}

¹Department of Otolaryngology-Head & Neck Surgery, University of Toronto, Toronto, ON, Canada; ²Institute of Biomedical Engineering, University of Toronto, Toronto, ON, Canada; ³KITE - Toronto Rehabilitation Institute, University Health Network, Toronto, ON, Canada; ⁴Division of Urology, Department of Surgery, St. Michael's Hospital, Toronto, ON, Canada; ⁵Department of Surgery, University of Toronto, Toronto, ON, Canada; ⁶WellSpring Research, Toronto, ON, Canada; ⁷Temerty Faculty of Medicine, University of Toronto, Toronto, ON, Canada; ⁸Li Ka Shing Knowledge Institute, St. Michael's Hospital, Toronto, ON, Canada

Cite as: Trac J, Lee J, Fok KH, et al. Development of a synchronous motion-tracking and video capture tool for flexible ureteroscopy. *Can Urol Assoc J* 2024;18(4):103-9. <http://dx.doi.org/10.5489/cuaj.8530>

Published online December 21, 2023

ABSTRACT

INTRODUCTION: Hand/instrument motion-tracking in surgical simulation provides valuable data to improve psychomotor skills and can serve as a formative evaluation tool. Motion analysis has been well-studied in laparoscopic surgery; however, there are essentially no studies looking at motion-tracking for flexible ureteroscopy (fURS), a common surgical procedure requiring hand dexterity and 3D spatial awareness. We aimed to design a synchronized motion-tracking and video capture system for fURS capable of collecting objective metrics for use in surgical skills training.

METHODS: Motion tracking of the ureteroscope was performed using a motion-tracking platform, inertial measurement units (IMUs), and an optical sensor. Position (x, y, z) and orientation (roll, pitch, yaw) of the ureteroscope handle, lever deflection, and translation of the scope insertion point were collected. Video capture of the operator's hands was collected with a Raspberry Pi camera. All peripherals were controlled on a Raspberry Pi 4 and synchronized to its system clock.

RESULTS: Our system demonstrated good accuracy in detecting translation of the ureteroscope in the x- and y-axes, and yaw, pitch and roll of the ureteroscope at discrete orientations of 0, ± 30 , ± 60 , and ± 90 degrees. Unique to fURS, deflection of the lever was captured by the difference in IMU static accelerations with good accuracy. The optical sensor detected translation of the ureteroscope at the insertion point with good precision and an average error of 5.51%.

CONCLUSIONS: We successfully developed a motion-tracking and video-capture system capable of collecting motion-analysis parameters unique to fURS. Future studies will focus on establishing the construct validity of this tool.

INTRODUCTION

Flexible ureteroscopy (fURS) is a common surgical procedure for the management of upper urinary tract pathologies.¹ Maneuvering a flexible ureteroscope efficiently and effectively is initially not intuitive to a junior learner, as this requires both hand dexterity and three-dimensional (3D) spatial awareness. Performing fURS requires coordination of psychomotor skills, and, at times, fine rotational and translational movement of the ureteroscope in multiple degrees of freedom (DOF). Studies have shown that a trainee must complete around 60 cases to achieve a good level of competence, and 100 cases for complication rates to plateau.²

Numerous URS surgical simulation platforms have been developed to allow surgical trainees to tune their skills outside of the operating room;³⁻⁵ however, there remains a lack of objective constructive feedback to the trainee during simulation study, particularly with respect to how they can improve their specific hand/instrument motions.

It is well-established that hand and instrument motion-tracking in surgical simulation can provide valuable educational information to the operator.^{6,7} Motion-tracking of psychomotor skills in laparoscopic surgery is well-studied. Technologies implemented for motion-tracking include electromagnetic tracking systems, infrared cameras, accelerometers, and optical sensors.⁷⁻¹⁰ Motion-analysis parameters (MAPs), such as operative time, path length, velocity, acceleration, and jerk of

KEY MESSAGES

- Hand/instrument motion-tracking in surgical simulation can provide valuable data to trainees to develop psychomotor skills.
- Our study outlines the development and validation of a motion-tracking and video-capture system for flexible ureteroscopy with unique metrics including lever deflection and scope translation at the insertion point.
- The collected metrics from our system has strong associations with categories used in validated evaluation checklists, such as the ureteroscopic global rating scale.

the instrument, have been reported to be able to distinguish between novice and expert laparoscopic operators.^{7,8,10-12} Heiliger et al implemented instrument motion-tracking for a laparoscopic training course with inertial measurement units (IMUs) and demonstrated an ability to examine the learning progress of medical students in an ex-vivo environment.¹³ Hardon et al delivered a laparoscopy training course with the integration of motion-tracking in its training goals paired with instant, objective feedback after each trial and reported an improvement in instrument-handling skills over time.¹⁴ Motion-tracking systems have the potential to serve as a formative evaluation tool by providing operators with feedback on how their psychomotor skills compare to operators of varying expertise and tracking learning progress over time.

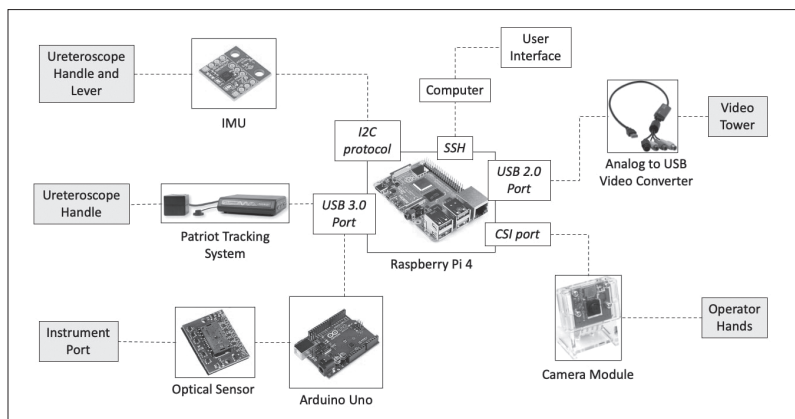


Figure 1. Diagram of connections between Raspberry Pi 4 and all system peripherals. The Pi has USB 2.0 and 3.0 ports, inter-Integrated Circuit (I2C) communication protocols, and a Camera Serial Interface (CSI) camera port. The Pi is controlled by the user remotely through a personal computer with Secure Shell Protocol (SSH).

Despite being well-established in laparoscopic training, there are limited studies that investigate motion-tracking in endoscopic procedures.¹⁵⁻¹⁷ Salvadó et al used an electromagnetic tracking system to collect motion-tracking data in semi-rigid ureteroscopy and reported correlations between an operator's MAPs (time taken, path length, numbers of movements) and assessment scores from validated checklists: the Global Rating Scale (GRS) and urethral checklist (UC).¹⁸ There are numerous simulators developed for fURS, such as URO Mentor™ (Symbionix Ltd., Israel) and Scope Trainer (Mediskills Ltd., U.K.); however, no URS simulators to date implement motion-tracking analysis feedback specifically for fURS.^{3,4,19-23}

Learner performance with fURS simulators have been traditionally assessed with validated checklists, such as the procedural-specific GRS adapted by Matsumoto et al for the endourologic environment.^{24,25} Checklist assessments rely on subjective expert observation and expert evaluator availability.^{7,8,26} Thus, designing a system that can provide objective data collection and feedback on an operator's instrument-handling technique is valuable. Such a system would allow novice fURS operators to develop their psychomotor skills in a safe, monitored, and controlled setting prior to exposure to real patients. The primary objective of our study was to design and validate a synchronized motion-tracking and video-capture system for fURS.

METHODS

The tool was designed for a single-use flexible ureterorenoscope, EU-Scope™ (Innovex Medical Co., Ltd., Shanghai, China). The tip deflection range is 275°. Institutional review board approval and written consent were not required, as no human subjects participated in the study.

The hardware components of the tool include: 1) a Raspberry Pi (Raspberry Pi, U.K.); 2) the Patriot motion-tracking system (Polhemus™, VT, U.S.);²⁷ 3) two IMUs (SparkFun Electronics, CO, U.S.); 4) an optical sensor (JACK Enterprises, TN, U.S.); 5) an Arduino Uno (Arduino Uno, Ivrea, Italy); 6) a Raspberry Pi camera; 7) an analog-to-USB video converter (Hauppauge, PA, U.S.); and 8) 3D printed housing. The software components include: 1) the Patriot firmware; and 2) the user interface with control scripts.

Hardware

RASPBERRY PI

The Raspberry Pi 4 interfaces with the motion-tracking and video-capture peripherals (Figure 1). It is a widely

available platform at a low cost (\$40 CAD) with many interfaces for sensors and cameras.

INERTIAL MEASUREMENT UNIT

Two IMUs were used to capture ureteroscope lever deflection. The tool implemented the MPU9250 IMU Breakout Board, which consists of a 3D accelerometer, 3D gyroscope, and 3D magnetometer that measure static acceleration, angular rotation, and magnetic field strength. The IMUs are attached onto the side of the lever and on the handle inferior to the lever to measure deflection through the difference in static acceleration (Figures 2A, 2B). The outputs are processed by 16-bit analog-to-digital converters (ADC). The sensitivity of the accelerometer can be set between 2 g force (g) to 16 g. When operating at the range from -1 g to +1 g, it has a sensitivity of 0.005°/LSB (least significant bit). An alternative sensor for capturing deflection of the ureteroscope is a potentiometer, which captures rotational movement, such as in a volume knob.

OPTICAL SENSOR

The PMW3360 motion sensor board implements a PMW3360DM-T2QU (PixArt Imaging, Taiwan) navigation gaming sensor. Movement in the x- and y-axes is detected by acquiring images and performing digital image correlation. The sensor is placed above the insertion point to measure ureteroscope translation along its longitudinal axis (Figures 2C, 3). A 16-bit output represents movement in counts per inch (CPI). The resolution can be programmed from a range of 100–12000 CPI (4–472 counts per mm). The frame rate is up to 12000 frames per second (fps). Optical sensors are commonly used in applications that require collection of translation. For example, they are used under gaming mice to translate movement of the mouse on the desk to move the computer cursor with high accuracy.

MICROCONTROLLER

The Arduino Uno interfaces the optical sensor with the Pi. The Arduino Serial Peripheral Interface (SPI) library was used to communicate with the optical sensor. The Arduino is versatile, cost-effective, and has open-source software (available at: <https://www.arduino.cc/en/software>).²⁸

PATRIOT SYSTEM

The Patriot motion-tracking system uses electromagnetic technology. Our tool employs one standard RX2 sensor on the ureteroscope handle (Figures 2A, 2B), which tracks six DOF to capture translational

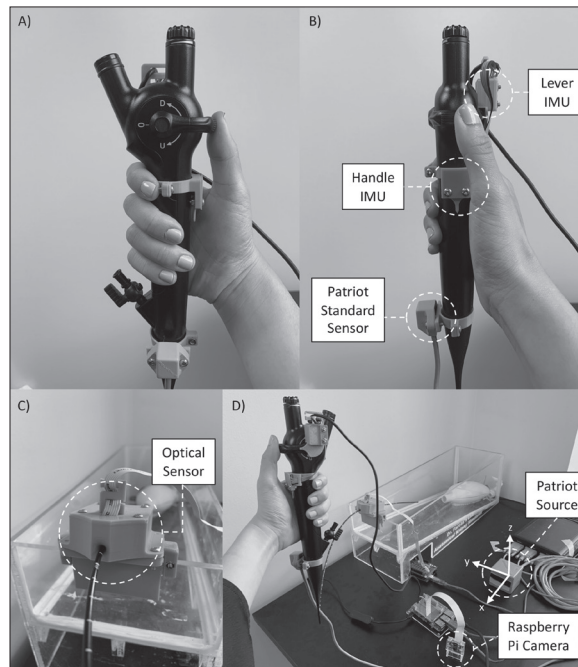


Figure 2. Complete motion-tracking and video-capture tool. (A) (B) Inertial measurement unit and Patriot standard sensor fitted onto the single-use flexible ureteroscope. (C) Optical sensor fitted to project above the insertion point of the ureteroscope onto a simulator box. (D) Complete view of tool with Patriot source (i.e., reference coordinates for x-, y-, and z-axes) and Raspberry Pi camera module pointing toward operator's hands.

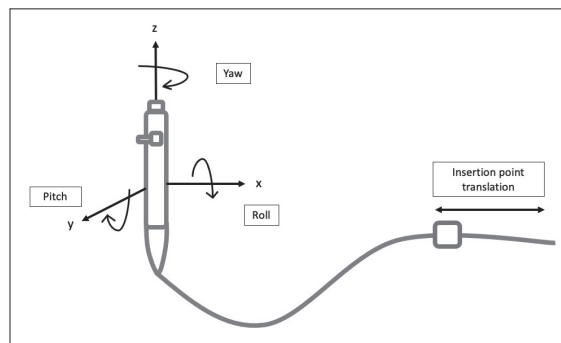


Figure 3. Illustration of the measurement of roll, pitch, and yaw in relation to the rotational movement of the ureteroscope and translation at the insertion point.

(forward-back, side-side, up-down) and rotational (roll, pitch, yaw) movements of the handle. Roll, pitch, and yaw is the rotation about the ureteroscope's longitudinal, vertical, and lateral axes, respectively (Figure 3). The Patriot system samples at a rate of 60 Hz. The field source defines the x-, y-, and z-axes of the sensor outputs. Its optimal working range is 90 cm (Figure 2D).

RASPBERRY PI CAMERA MODULE

The Raspberry Pi v2 camera module is powered by a IMX219 (Sony, Japan) 8-megapixel sensor. It records the operator's hand movements (Figure 2D). It attaches

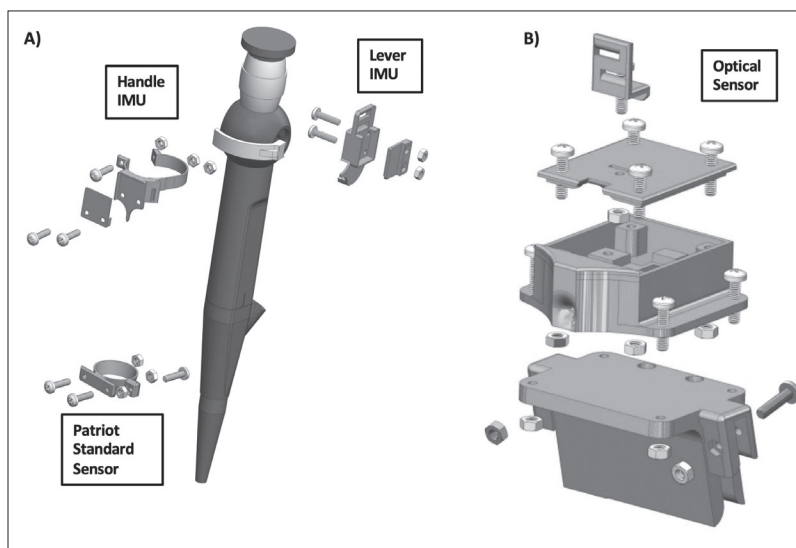


Figure 4. Diagrams of sensor mounts and components used in the motion-tracking system. (A) Mounts for two internal measurement units and Patriot sensor used on the ureterscope. (B) Attachment clip (bottom) and the housing (center) for the optical sensor.

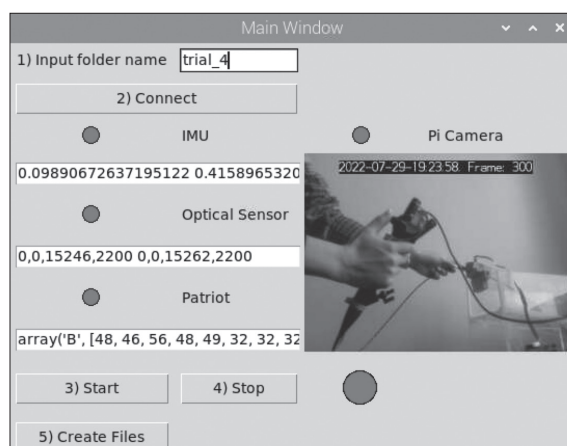


Figure 5. Graphical user interface to control the system with buttons to connect all peripherals and start and stop data collection with the Raspberry Pi. The user interface refreshes every 100th data frame to indicate ongoing data collection and video capture of the operator hands.

to the Pi camera port via ribbon cable. The maximum resolution is 1920x1080 pixels at 30 fps.

ANALOG-TO-USB VIDEO GRABBER

We used an analog to digital video converter, USB-Live 2, to capture endoscopic video. The analog (s-video) output from the video tower is collected, digitized and transmitted to the Pi at a resolution up to 1280x720 at 30 fps.

HOUSING FOR ALL PERIPHERALS

Housings for peripheral sensors were designed using a computer-aided design software, SolidWorks 2021

(Dassault Systèmes, San Diego, CA, U.S.), and a 3D-printer, Ender 3 Pro (Creality, Shenzhen, China). The IMU housing consists of: 1) a press fit attachment to the lever; and 2) a circular attachment to the handle inferior to the lever (Figure 4). The Patriot sensor housing was attached to the inferior aspect of the ureterscope's handle with a circular attachment. The optical sensor housing was positioned superior to the instrument port, with an opening for the sensor to acquire images over the tunnel for the ureterscope. Except for the Patriot sensor, which was already self-contained, all housings were designed with a cover for water protection.

Software

PYTHON USER APPLICATION

A user application was developed using the Python Tkinter package (Python Software Foundation, Wilmington, U.S.) which coordinates synchronous data collection (Figure 5).

MOTION-TRACKING DATA COLLECTION

The optical sensor is polled by the Arduino at a rate of 66 Hz. The data is sent to the Pi via serial communication. The PyUSB package was used to read from and write to the Patriot system (available at: <https://github.com/pyusb/pyusb>). IMU data was collected using the open-source mpu9250-jmdev Python package, developed by Jeferson Menegazzo.²⁹ All data from the sensors were sampled at an average rate of 25 Hz by the Pi and saved with the Pi system's timestamps to a ".csv" file for post-processing.

VIDEO-CAPTURE COLLECTION

The video images captured by the camera module were displayed on the graphical user interface (Figure 4). The video captured by the analog-to-USB video converter was sent to the Pi via the USB 2.0 port. The Fast Forward Motion Picture Experts Group (FFmpeg) library (available at: <https://ffmpeg.org/ffmpeg.html>) was used to record the captured video at a frame rate of 25 fps. The video was encoded using H264 compression and saved as an ".avi" file.

Testing

OPTICAL SENSOR

Translation of the ureterscope was measured by the optical sensor at the insertion point. A series of 10 trials were conducted for distances of 25, 50, and 100 mm

along the longitudinal axis of the ureteroscope. The actual translation was measured by an electronic caliper.

IMU AND PATRIOT

The translation and orientation of the ureteroscope handle was measured by the Patriot system. The deflection of the ureteroscope lever was measured by the IMUs on the lever and handle. The Patriot and IMUs are well-validated. Therefore, tests were conducted to demonstrate that the sensors were capturing movement as expected.

Translation of the ureteroscope was tested by moving 300 mm along the x- and y-axes of the working space. The Patriot source, which defines the reference axes, was placed approximately 300 mm away from the simulator box, such that the working space included the area in front of the simulator box (Figure 2). Roll, pitch, and yaw of the ureteroscope handle were tested within the -90 to $+90^\circ$ range by orienting the ureteroscope at $0, \pm 30, \pm 60$, and $\pm 90^\circ$ with reference to a 30-60-90 triangle. The deflection of the lever was tested within its full range.

RESULTS

Rotation of the ureteroscope is depicted in Figures 6A–6C as discrete orientation changes at $0, \pm 30, \pm 60$, and $\pm 90^\circ$ along the yaw, pitch, and roll axes. Negative orientation data was shifted to be in the positive range (0 – 360°). Translation of the ureteroscope 300 mm in the x- and y-axes is depicted in Figure 6D as discrete positional changes. The deflection of the lever up, down, and back to neutral is depicted in Figure 7. The data was post-processed with a Butterworth filter with a normalized cutoff frequency of 0.2.

The optical sensor demonstrated an average error of 5.51% across all three distances. The percent error corresponds to a discrepancy between the actual distance measured and the distance detected by the sensor, which was 1.37–5.37 mm. The highest standard deviation across all trials was 2.02 mm (Table 1).

DISCUSSION

We developed a novel motion-tracking and video-capture tool for fURS. We demonstrated good accuracy in capturing the movement and rotation of the ureteroscope handle. We also captured the operator's manipulation of the ureteroscope's lever, which is associated with the deflection of the ureteroscope tip. The tool's ability to capture translation of the ureteroscope at the insertion point was tested and demonstrated good accuracy and precision. The tool was able to simultan-

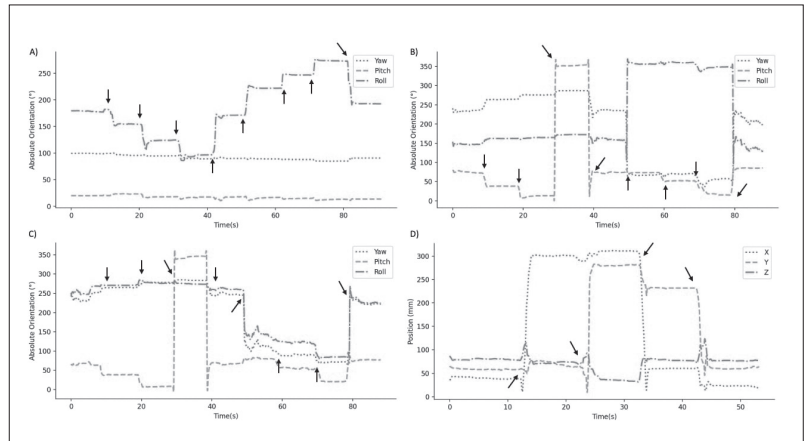


Figure 6. Position and absolute orientation data collected from the Polhemus Patriot sensor attached to the ureteroscope handle. Orientation data when rotating ureteroscope (A) in the z-axis (roll); (B) in the y-axis (pitch) from 5 – 365 degrees; (C) in the x-axis (yaw). (D) Position data when translating scope 300 mm along the x-axis (+), y-axis (+), x-axis (–), and y-axis (–) every 10 seconds.

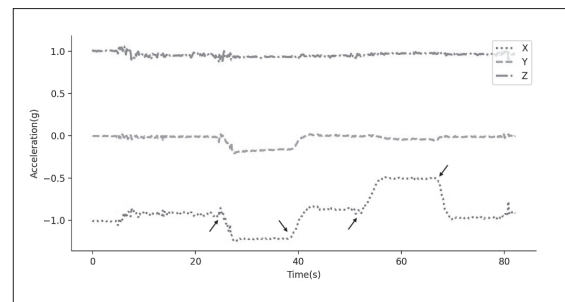


Figure 7. Difference in static acceleration of the inertial measurement units (IMUs) attached to the lever of the ureteroscope when moving the lever up, down to neutral, down, and up to neutral (full range of motion) to the IMU attached to the handle. Lever motion is associated with 275° deflection of the ureteroscope tip.

Table 1. Optical sensor accuracy testing for measurement of translation of ureteroscope along longitudinal axis

	Electronic caliper distance (mm)	Sensor reported mean distance \pm SD (mm)	Error (%)
Optical sensor	24.93	23.56 \pm 1.30	1.37 (5.49)
	50.22	47.37 \pm 0.80	2.85 (5.68)
	100.42	95.05 \pm 2.02	5.37 (5.35)
Average error			3.20 (5.51)

SD: standard deviation.

eously video-capture the operator's hand movements. System synchronization was confirmed visually between the video playback and the motion-tracking output system timestamps.

The testing demonstrates the ability of the tool to capture MAPs similar to those reported in previous studies for laparoscopy and semi-rigid ureteroscopy. Salvadó et al collected hand-motion data for semi-rigid ureteroscopy and reported MAPs, such as time to task completion and number of hand movements, as discriminatory between expert and novice operators.¹⁸ Similarly, our tool records the time taken to complete a task, and goes well beyond a simple count of hand movements.

Van Empel et al used motion-tracking to analyze a knot square-tying task in laparoscopy and reported that the 3D space (volume, mm³) used by the operator's hand was significantly smaller in expert operators.¹¹ Similarly, our tool can extrapolate total working space through positional changes of the handle. Our tool also had a similar average error in detecting translation of a laparoscopic simulator, which used an optical sensor at the insertion point of the instrument (5.51% in our study vs. 6.75% and 5.4% for right- and left-handed laparoscopic instruments, respectively).³⁰

Our system is designed specifically for fURS training; and therefore, there were additional MAPs we sought to capture. First, movement of the ureteroscope handle is dictated by the dominant hand; however, the non-dominant hand is often responsible for guiding the ureteroscope tip into the access sheath. Operators can manipulate the instrument at this point independent of the ureteroscope handle. Our tool can accurately and precisely report translation of the ureteroscope at the insertion point by placement of the optical sensor above it.

Second, compared to laparoscopy, the manipulation of the ureteroscope lever plays a crucial role in visualization of anatomy and the ability to complete a task. Our tool captures the extent of lever manipulation through the difference in static acceleration of the IMUs attached to the lever and handle. The rotation of the ureteroscope handle also factors into visualization of structures. Koo et al reported preliminary findings where roll of the ureteroscope handle was less pronounced in experts compared to novices using the Patriot system.⁵ Our tool reports handle rotation to a good level of accuracy about all three axes. With these metrics, we have developed a tool capable of robustly capturing clinically relevant movements in fURS.

Virtual reality (VR) simulators are becoming increasingly popular in the surgical simulation space. Uro Mentor is an example of a simulator for both rigid and flexible ureteroscopy which incorporates motion-tracking analysis; however, VR systems can cost upwards to \$70000 CAD.³¹ In addition, the simulator requires space in an operating room and various equipment,

including a mannequin, and requires the operator to wear a bulky headpiece.³² There is a high level of simulation achieved with VR but at additional costs and resources, which may only be accessible to large endourologic centres.

A strength of our system is that its motion-tracking and video-capture data has strong associations with categories used in validated evaluation checklists, such as the ureteroscopic GRS.²⁴ For example, the "Time and Motion" category assesses optimization of time and number of movements made, which can be identified from time to task completion and number of unnecessary movements identified on video-capture. Two categories, "Instrument Handling" and "Handling of Endoscope," assess for smooth movements and a well-centered ureteroscope. We can assess the smoothness of the operator's movements by calculating the number of directional changes made with respect to the ureteroscope's position. We can determine how often the ureteroscope's center changes by calculating the number of orientation changes in each DOF.

We anticipate that our tool will eventually be able to go beyond the current validated checklists in assessing learner skill acquisition because it is able to accurately and objectively capture all relevant DOF associated with fURS. In a simulation setting, this tool has the potential to inform the learner of which exact movements are unnecessary. By providing this feedback immediately and objectively without an expert instructor watching, we are hopeful that our tool will shorten the fURS learning curve.

Limitations

There are several limitations to our system. The system integrates Patriot, a commercial system that has accurate motion-tracking capabilities, but adds a substantial cost; however, Koo et al demonstrate that the Patriot has capability to distinguish between expert and novice operators in fURS when looking at differences in roll of the ureteroscope.⁵ The novel metrics gathered in the system (i.e., insertion point translation, lever deflection) use off-the-shelf components (i.e., IMU, optical sensors), making it more accessible for interested researchers to replicate these components.

Due to our focus on motion analysis, the system does not yet integrate force measurements, which is important when learning how to properly handle tissue in endoscopic procedures;³³ however, haptic feedback is more relevant for semi-rigid URS rather than flexible URS, which has limited tactile feedback.³¹

The system also cannot assess non-technical skills, such as leadership and situational awareness.

Goldenberg et al and Brunckhorst et al both mention this limitation in most methods of assessment for surgical skills.^{22,23}

Our system will be the subject of future studies. The next step would be to implement a study that assesses the system's construct validity. Specifically, it would be important to determine which MAPs specific to fURS can discriminate between expert and novice operators. Ultimately, would the tool have potential to serve as an objective measure of performance and provide trainees with insight into areas for improvement?

CONCLUSIONS

We have designed a motion-tracking and video-capture system for fURS. It is capable of collecting novel MAPs deemed important in fURS. The next step will be establishing the construct validity of the system for a particular ureteroscopy task, such as visualization of calyces.

COMPETING INTERESTS: The authors do not report any competing personal or financial interests related to this work.

ACKNOWLEDGEMENT: The authors would like to thank Unity Health Toronto for funding the study through the Keenan Research Summer Student (KRSS) Program.

This paper has been peer-reviewed.

REFERENCES

- Alenezi H, Denstedt JD. Flexible ureteroscopy: Technological advancements, current indications and outcomes in the treatment of urolithiasis. *Asian J Urol* 2015;2:133-41. <https://doi.org/10.1016/j.ajur.2015.06.002>
- Quirke K, Aydin A, Brunckhorst O, et al. Learning curves in urolithiasis surgery: A systematic review. *J Endourol* 2018;32:1008-20. <https://doi.org/10.1089/end.2018.0425>
- Simbionix Ltd. URO Mentor. 2014. Available at: <https://simbionix.com/simulators/uro-mentor/>. 2014; Accessed August 22, 2022
- Medskills Ltd. Medskills Standard Scope Trainer - SST. Available at: <https://www.medskills.com/products/scope-trainer/>. Accessed August 22, 2022
- Koo S, Fok K, Seo N, et al. Motion analysis in endoscopic surgery: Development of an enhanced simulation platform to aid in resident training. *J Urol* 2020;203:e509. <https://doi.org/10.1097/JU.0000000000000878>
- Farcas MA, Trudeau MO, Nasr A, et al. Analysis of motion in laparoscopy: The deconstruction of an intra-corporeal suturing task. *Surg Endosc* 2017;31:3130-39. <https://doi.org/10.1007/s00464-016-5337-4>
- Nasr A, Carrillo B, Gerstle JT, et al. Motion analysis in the pediatric laparoscopic surgery (PLS) simulator: Validation and potential use in teaching and assessing surgical skills. *J Pediatr Surg* 2014;49:791-4. <https://doi.org/10.1016/j.jpedsurg.2014.02.063>
- Moorthy K, Munz Y, Dosis A, et al. Bimodal assessment of laparoscopic suturing skills: Construct and concurrent validity. *Surg Endosc* 2004;18:1608-12. <https://doi.org/10.1007/BF02637130>
- Chmarra MK, Bakker NH, Grimbergen CA, et al. TrEndo, a device for tracking minimally invasive surgical instruments in training setups. *Sens Actuator A Phys* 2006;126:328-34. <https://doi.org/10.1016/j.sna.2005.10.040>
- Ebina K, Abe T, Higuchi M, et al. Motion analysis for better understanding of psychomotor skills in laparoscopy: Objective assessment-based simulation training using animal organs. *Surg Endosc* 2021;35:4399-416. <https://doi.org/10.1007/s00464-020-07940-7>
- van Empel PJ, van Rijssen LB, Commandeur JP, et al. Validation of a new box trainer-related tracking device: the TrEndo. *Surg Endosc* 2012;26:2346-52. <https://doi.org/10.1007/s00464-012-2187-6>
- Yamaguchi S, Yoshida D, Kenmatsu H, et al. Objective assessment of laparoscopic suturing skills using a motion-tracking system. *Surg Endosc* 2011;25:771-5. <https://doi.org/10.1007/s00464-010-1251-3>
- Heiliger C, Andrade D, Geister C, et al. Tracking and evaluating motion skills in laparoscopy with inertial sensors. *Surg Endosc* 2023;37:5274-84. <https://doi.org/10.1007/s00464-023-09983-y>
- Hardon SF, van Gastel LA, Horemans T, et al. Assessment of technical skills based on learning curve analyses in laparoscopic surgery training. *Minim Invasive Surg* 2021;170:831-40. <https://doi.org/10.1016/j.surg.2021.04.024>
- Obstein KL, Patil VD, Jayender J, et al. Evaluation of colonoscopy technical skill levels by use of an objective kinematic-based system. *Gastrointest Endosc* 2011;73:315-21. <https://doi.org/10.1016/j.gie.2010.09.005>
- Vilmann AS, Lachenmeier C, Svendsen MBS, et al. Using computerized assessment in simulated colonoscopy: A validation study. *Endosc Int Open* 2020;8:E783-91. <https://doi.org/10.1055/a-1132-5259>
- Colella S, Søndergaard Svendsen MB, Konge L, et al. Assessment of competence in simulated flexible bronchoscopy using motion analysis. *Respiration* 2015;89:155-61. <https://doi.org/10.1159/000369471>
- Salvado JA, Oyanedel F, Sepúlveda S, et al. Validation of a high-fidelity model in ureteroscopy incorporating hand motion analysis. *Int Urol Nephrol* 2015;47:1265-69. <https://doi.org/10.1007/s11255-015-1023-z>
- Al-Jabir A, Aydin A, Abe T, et al. Validation of the advanced scope trainer for flexible ureterorenoscopy training. *Urology* 2017;110:45-50. <https://doi.org/10.1016/j.urology.2017.07.047>
- Blankstein U, Lantz AG, D'A Honey RJ, et al. Simulation-based flexible ureteroscopy training using a novel ureteroscopy part-task trainer. *Can Urol Assoc J* 2015;9: 331-5. <https://doi.org/10.5489/cuaj.2811>
- Villa L, Somani BK, Sener TE, et al. Comprehensive flexible ureteroscopy (FURS) simulator for training in endourology: The K-box model. *Cent European J Urol* 2016;69:118-20. <https://doi.org/10.5173/cej.2016.710>
- Goldenberg M, Ordon M, Honey JRD, et al. Objective assessment and standard setting for basic flexible ureterorenoscopy skills among urology trainees using simulation-based methods. *J Endourol* 2020;34:495-501. <https://doi.org/10.1089/end.2019.0626>
- Brunckhorst O, Aydin A, Abboudi H, et al. Simulation-based ureteroscopy training: A systematic review. *J Surg Educ* 2015;72:135-43. <https://doi.org/10.1016/j.jsurg.2014.07.003>
- Matsumoto ED, Hamstra SJ, Radomski SB, et al. A novel approach to endourological training: Training at the Surgical Skills Center. *J Urol* 2001;166:1261-6. [https://doi.org/10.1016/S0022-5347\(05\)65749-7](https://doi.org/10.1016/S0022-5347(05)65749-7)
- Martin JA, Regehr G, Reznick R, et al. Objective structured assessment of technical skill (OSATS) for surgical residents. *Br J Surg* 1997;84:273-8. <https://doi.org/10.1046/j.1365-2168.1997.02502.x>
- Hu D, Liu T, Wang X. Flexible ureteroscopy training for surgeons using isolated porcine kidneys in vitro. *BMC Urol* 2015;15. <https://doi.org/10.1186/s12894-015-0067-9>
- Polhemus. Patriot. Available at: <https://polhemus.com/motion-tracking/all-trackers/patriot>. 2008. Accessed August 22, 2022
- Arduino. Arduino Software. Available at: <https://www.arduino.cc/en/software>. Accessed August 22, 2022
- Menegazzo J, von Wangenheim A. MPU-9250 Sensors Data Collect. Available at: <https://github.com/Intelligent-Vehicle-Perception/MPU-9250-Sensors-Data-Collect/>. 2022. Accessed August 22, 2022
- Gavrilovic B, Fahy AS, Carrillo B, et al. Development of an open-source laparoscopic simulator capable of motion and force assessment: High tech at low cost. *J Laparoendosc Adv Surg Tech* 2018;28:1253-60. <https://doi.org/10.1089/lap.2018.0126>
- Knoll T, Trojan L, Haecker A, et al. Validation of computer-based training in ureterorenoscopy. *BJU Int* 2005;95:1276-9. <https://doi.org/10.1111/j.1464-410X.2005.05518.x>
- Michel MS, Knoll T, Kohrmann KU, et al. The URO mentor: development and evaluation of a new computer-based interactive training system for virtual life-like simulation of diagnostic and therapeutic endourological procedures. *BJU Int* 2002;89:174-7. <https://doi.org/10.1046/j.1464-4096.2001.01644.x>
- Kaler KS, Lama DJ, Safiullah S, et al. Ureteral access sheath deployment: How much force is too much? Initial studies with a novel ureteral access sheath force sensor in the porcine ureter. *J Endourol* 2019;33:712-8. <https://doi.org/10.1089/end.2019.0211>

CORRESPONDENCE: Dr. Jessica Trac, Temerty Faculty of Medicine, Toronto, ON, Canada; jessica.trac@mail.utoronto.ca